

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282


Date: 09/16/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:31
INTERNAL STANDARD	VERIFIED	12:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:31
BLANK TEST	0.00	12:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:32
BLANK TEST	0.00	12:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:33
BLANK TEST	0.00	12:34

26-37577

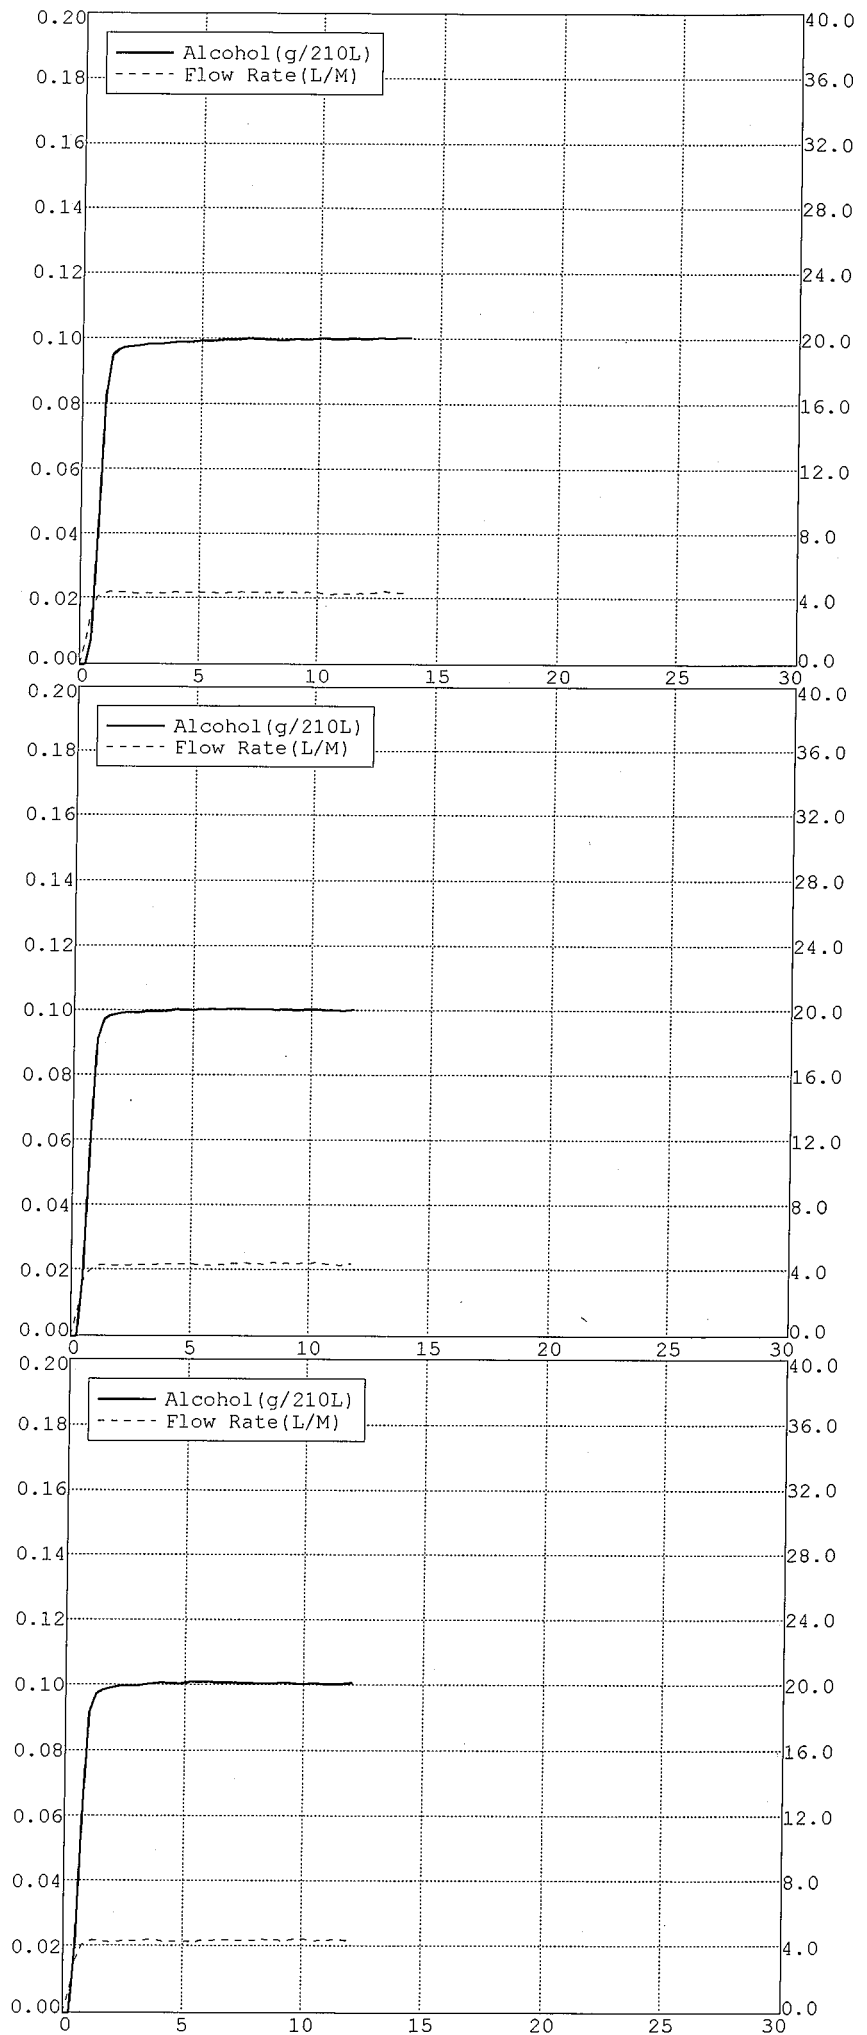

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 09/16/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:43
INTERNAL STANDARD	VERIFIED	12:43
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:43
BLANK TEST	0.00	12:44
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:44
BLANK TEST	0.00	12:45
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:45
BLANK TEST	0.00	12:46

26-37577

