

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 03/31/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:43
INTERNAL STANDARD	VERIFIED	12:43
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:43
BLANK TEST	0.00	12:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:44
BLANK TEST	0.00	12:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	12:46
BLANK TEST	0.00	12:46

26-12182

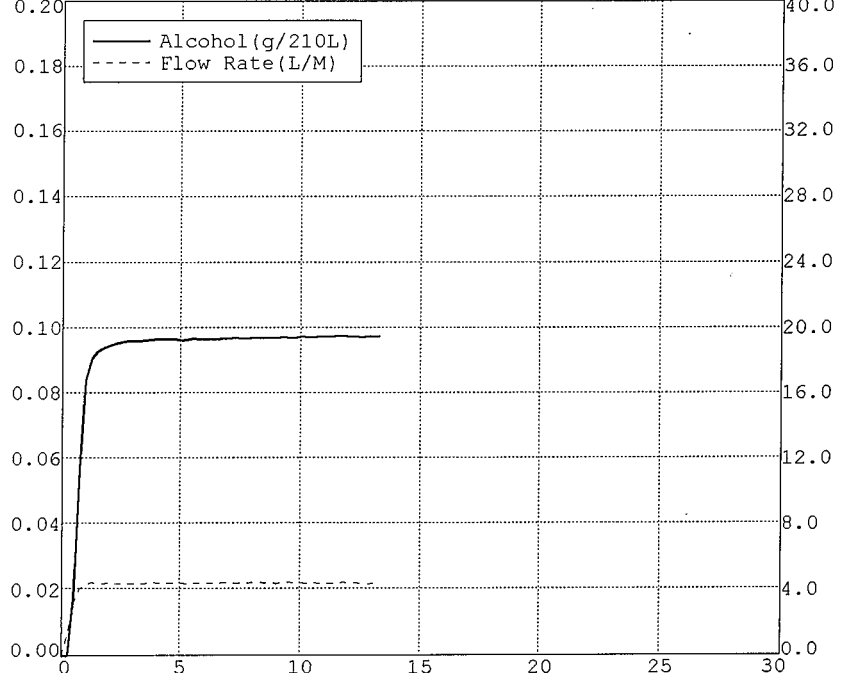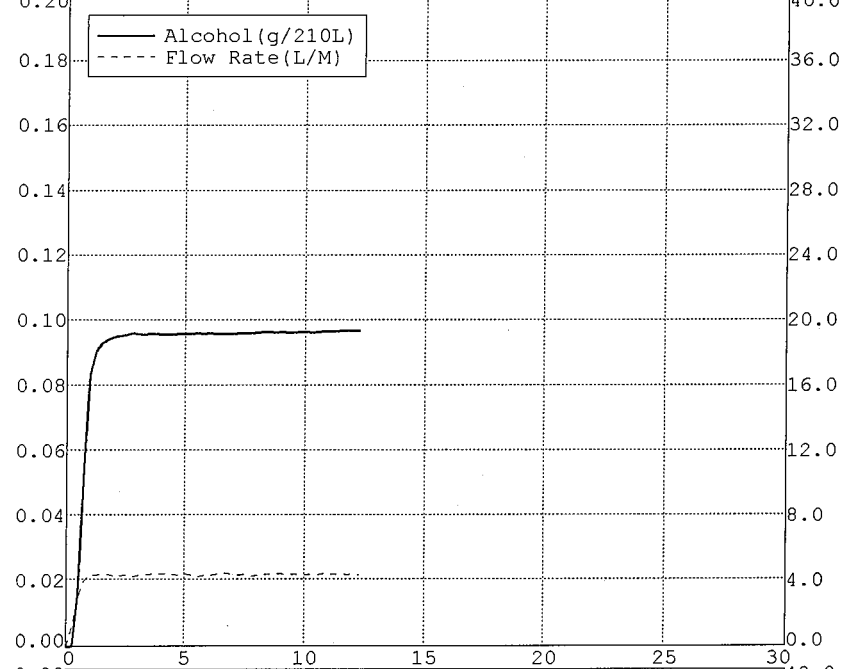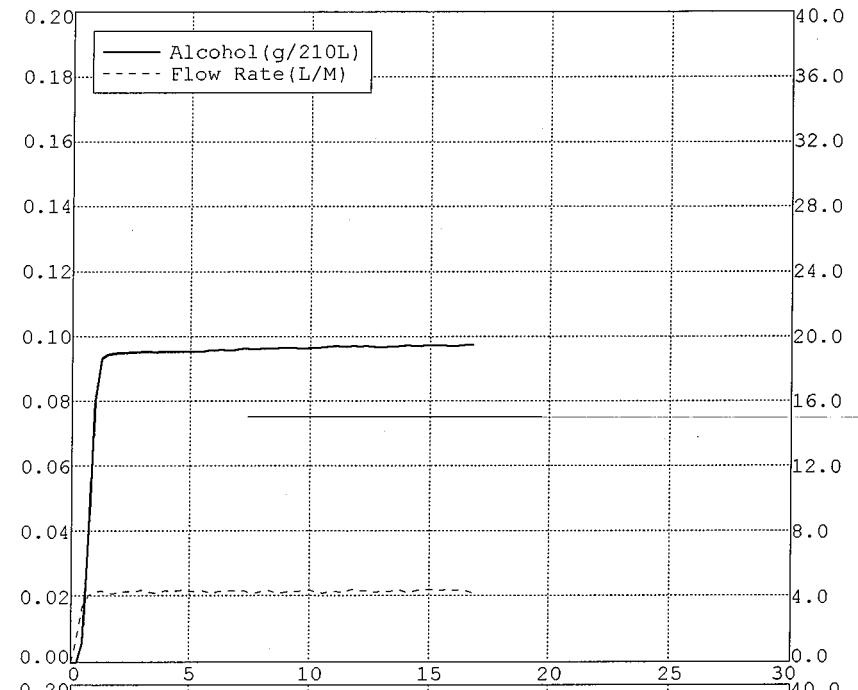

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 03/31/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:49
INTERNAL STANDARD	VERIFIED	12:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:50
BLANK TEST	0.00	12:51
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:51
BLANK TEST	0.00	12:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:52
BLANK TEST	0.00	12:53

26-12182

