

SOLUTION CHANGE

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 04/01/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:50
INTERNAL STANDARD	VERIFIED	10:50
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:50
BLANK TEST	0.00	10:51
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:51
BLANK TEST	0.00	10:52
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:52
BLANK TEST	0.00	10:53

26-12195

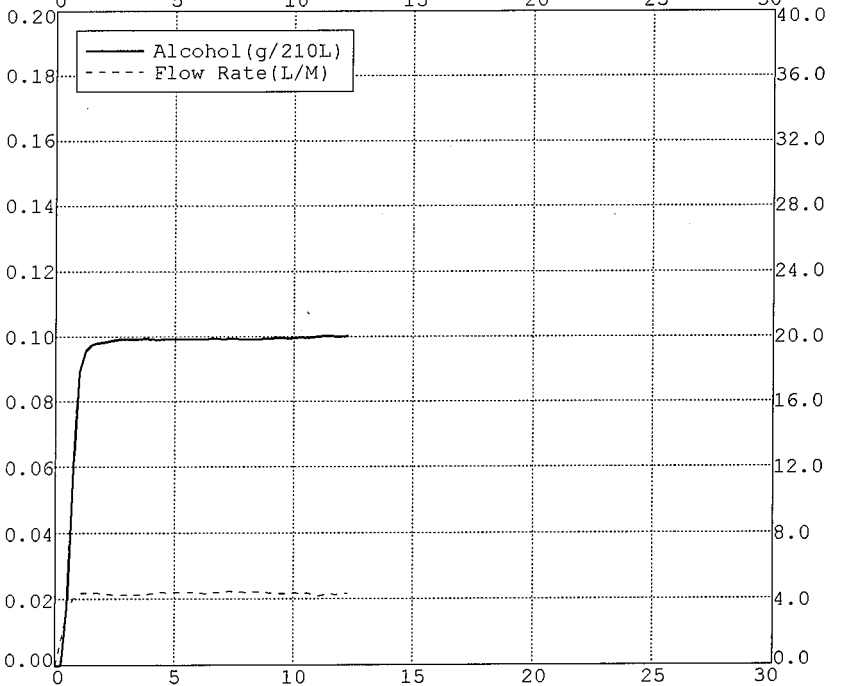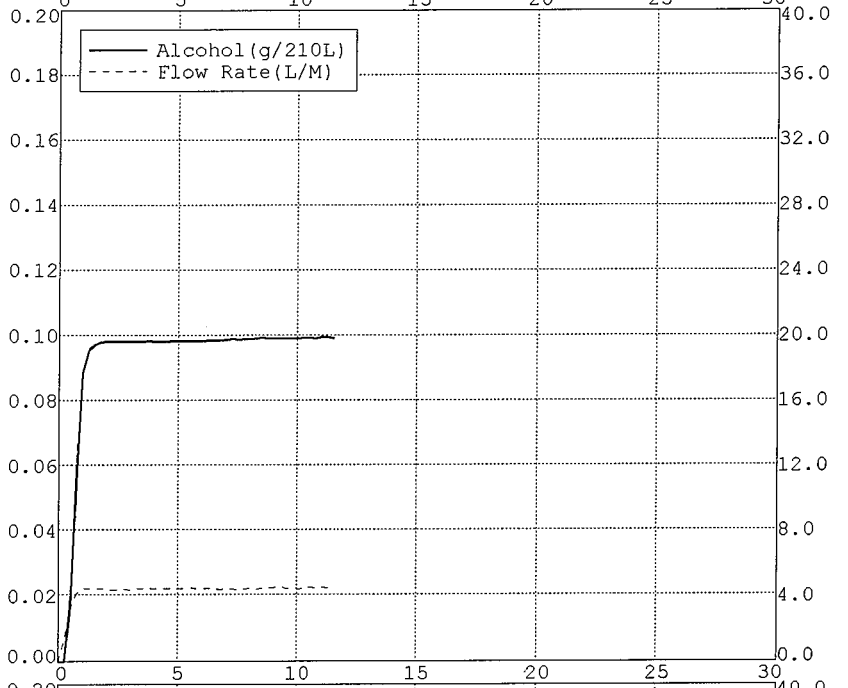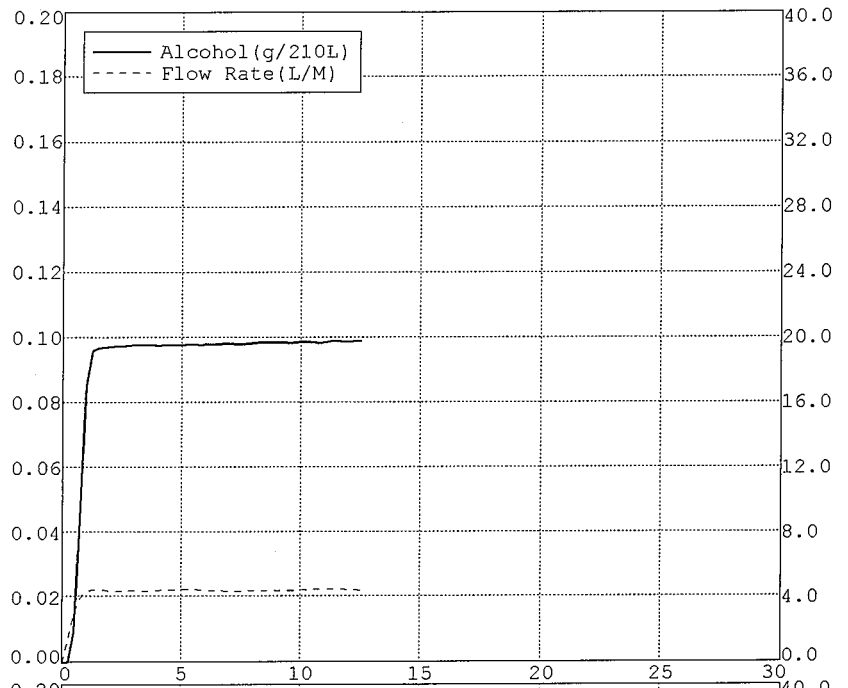

SOLUTION CHANGE

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 04/01/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:51
INTERNAL STANDARD	VERIFIED	10:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:51
BLANK TEST	0.00	10:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:52
BLANK TEST	0.00	10:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:54
BLANK TEST	0.00	10:54

26-12195

