

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 04/21/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:19
INTERNAL STANDARD	VERIFIED	13:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:20
BLANK TEST	0.00	13:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:21
BLANK TEST	0.00	13:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	13:22
BLANK TEST	0.00	13:23

26-15279

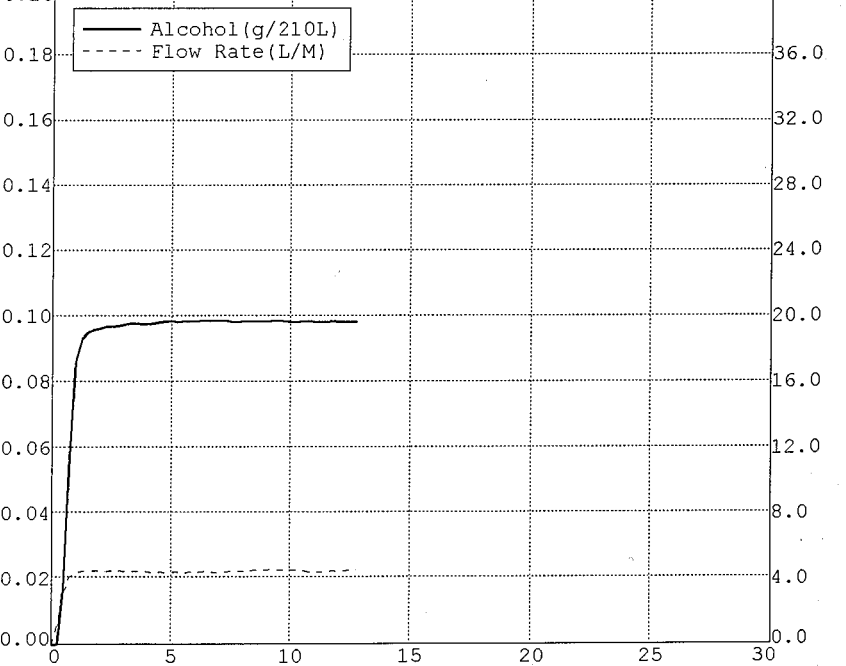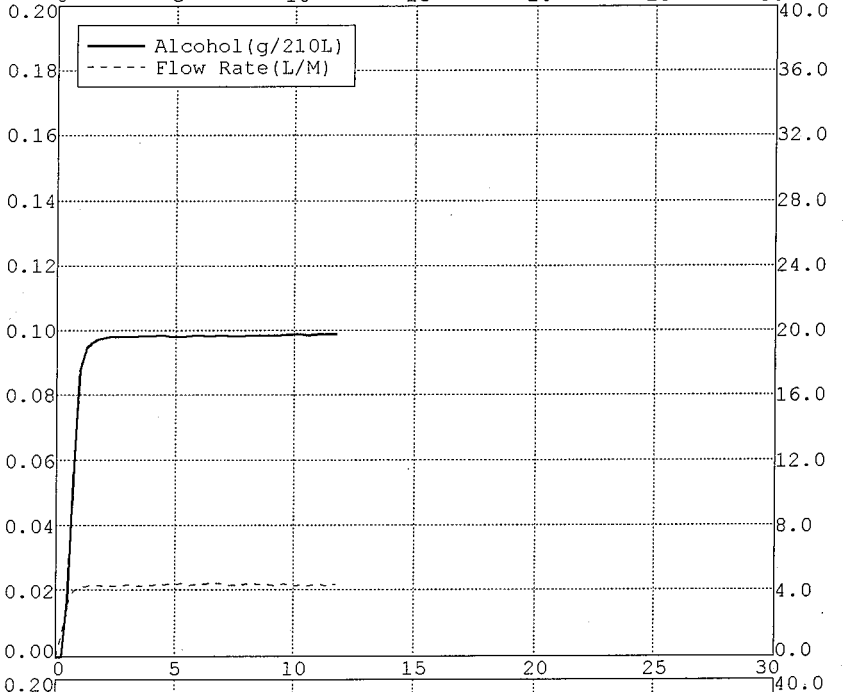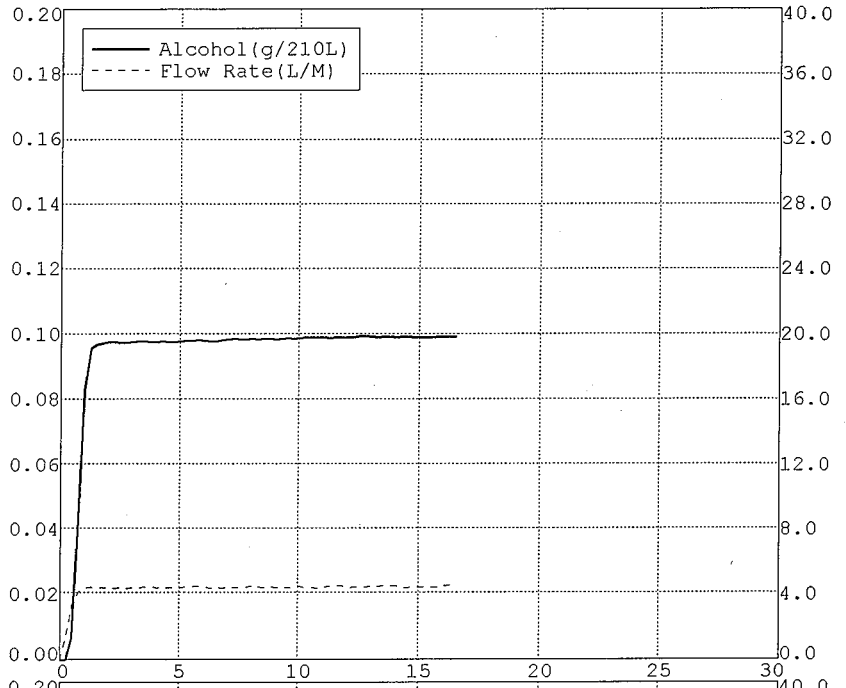

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 04/21/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:23
INTERNAL STANDARD	VERIFIED	13:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:23
BLANK TEST	0.00	13:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:25
BLANK TEST	0.00	13:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	13:26
BLANK TEST	0.00	13:26

26-15279

