

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 04/28/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:27
INTERNAL STANDARD	VERIFIED	14:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:27
BLANK TEST	0.00	14:28
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	14:28
BLANK TEST	0.00	14:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:30
BLANK TEST	0.00	14:30

26-16549

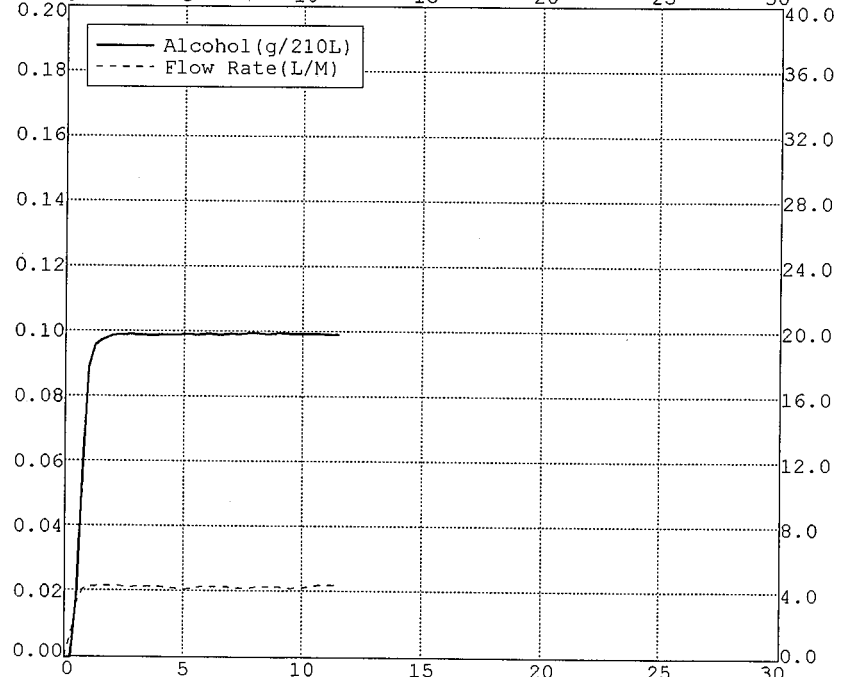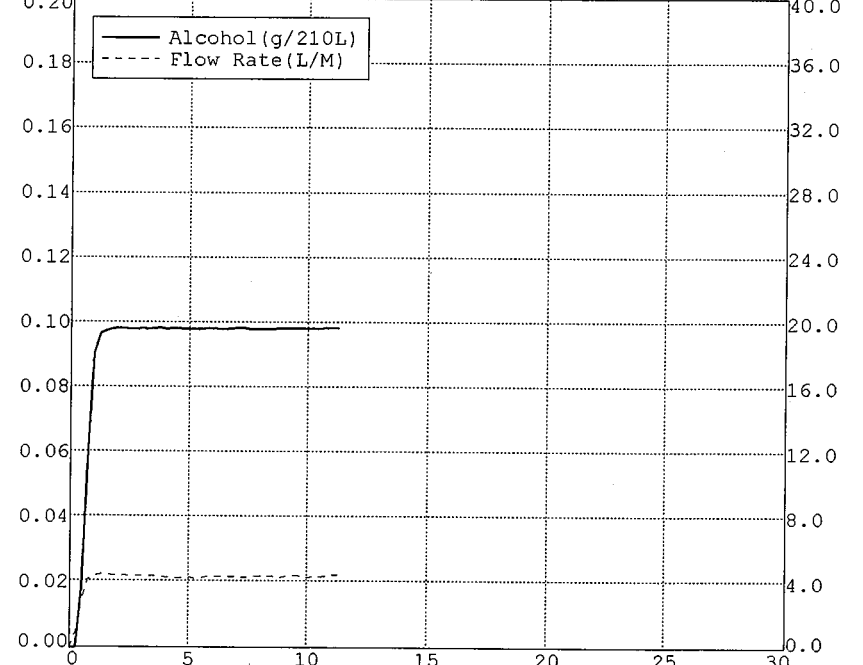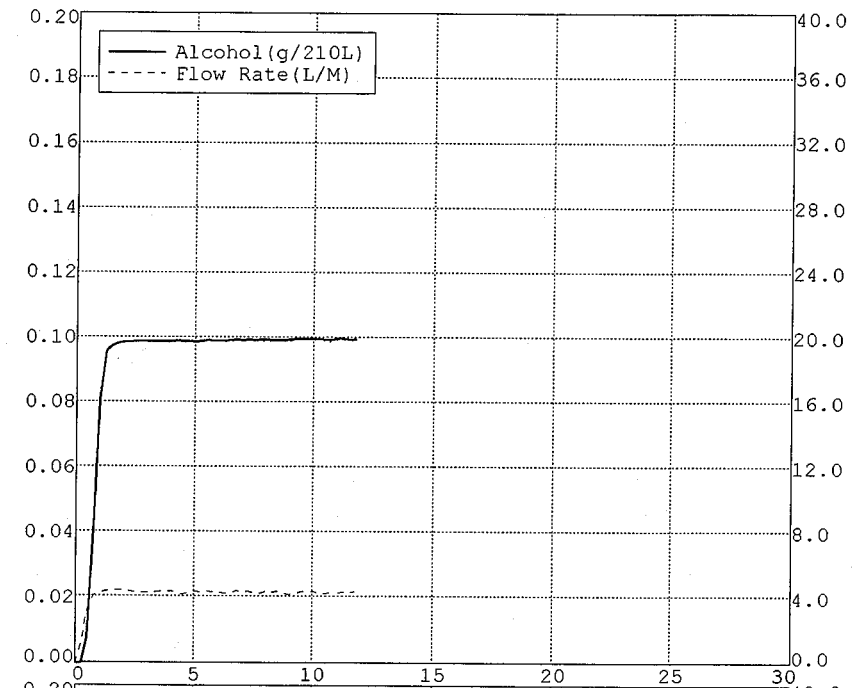

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 04/28/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:19
INTERNAL STANDARD	VERIFIED	14:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:20
BLANK TEST	0.00	14:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:21
BLANK TEST	0.00	14:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:22
BLANK TEST	0.00	14:23

26-16519

