

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 06/02/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:23
INTERNAL STANDARD	VERIFIED	11:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:23
BLANK TEST	0.00	11:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:24
BLANK TEST	0.00	11:25
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:25
BLANK TEST	0.00	11:26

26-21606

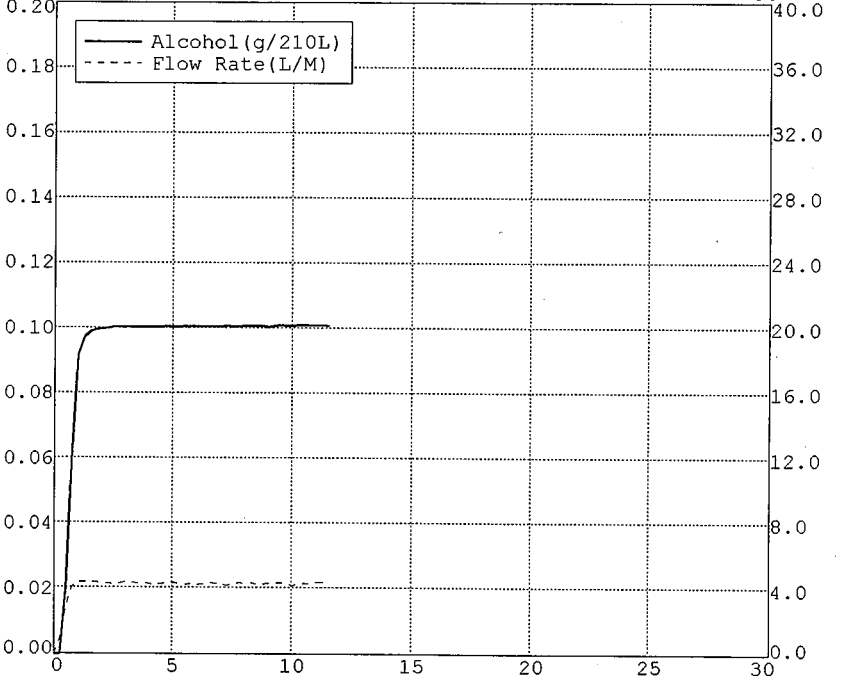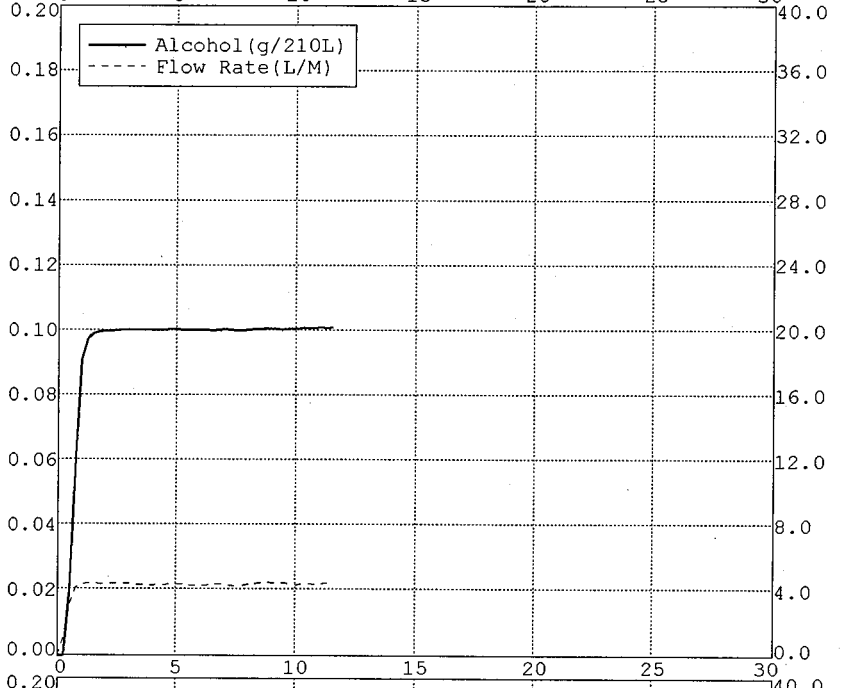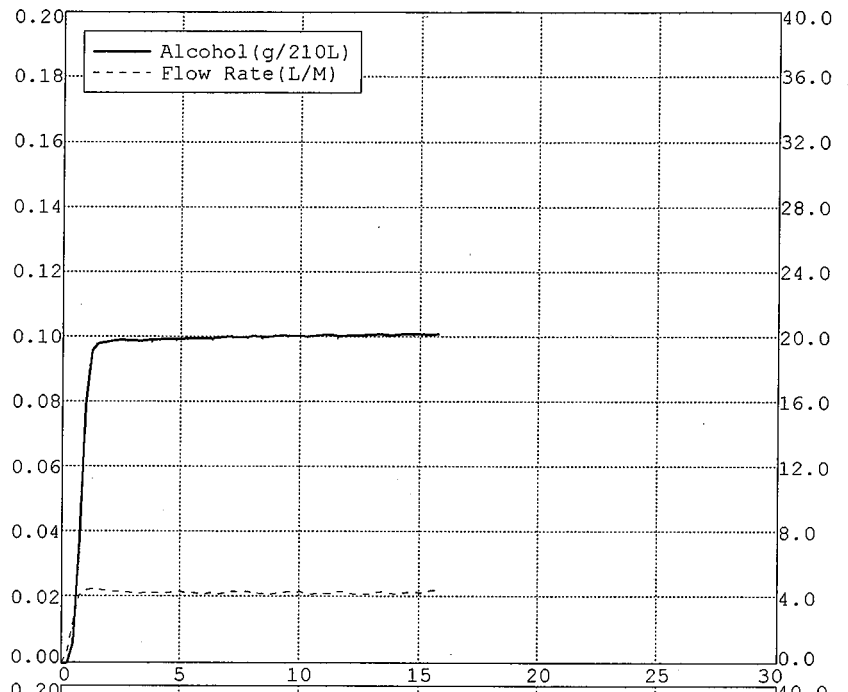

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 06/02/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:23
INTERNAL STANDARD	VERIFIED	11:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:23
BLANK TEST	0.00	11:24
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:24
BLANK TEST	0.00	11:25
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:26
BLANK TEST	0.00	11:26

26-21606

