

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 06/09/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:14
INTERNAL STANDARD	VERIFIED	10:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:15
BLANK TEST	0.00	10:16
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:16
BLANK TEST	0.00	10:17
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:17
BLANK TEST	0.00	10:18

26-22984

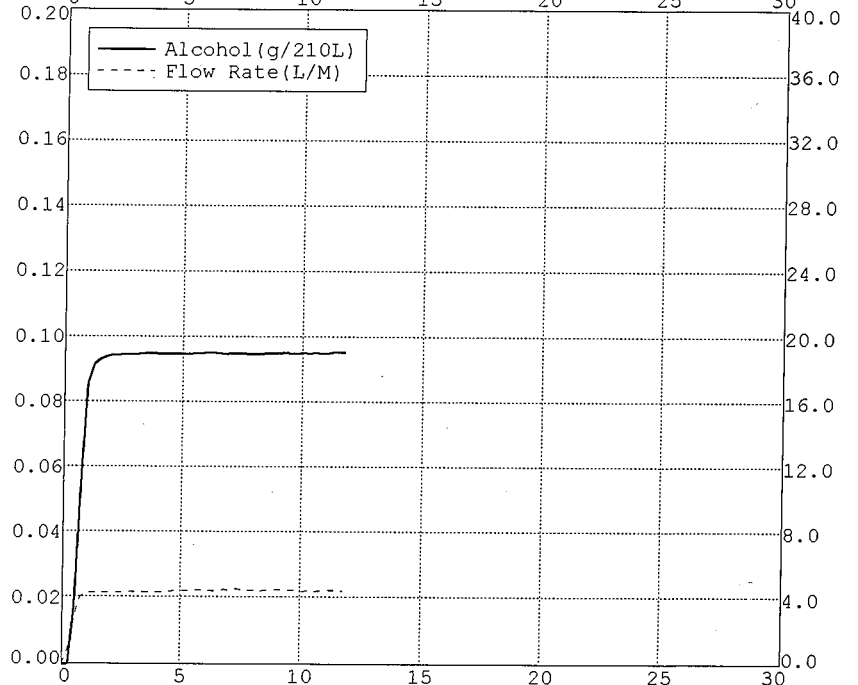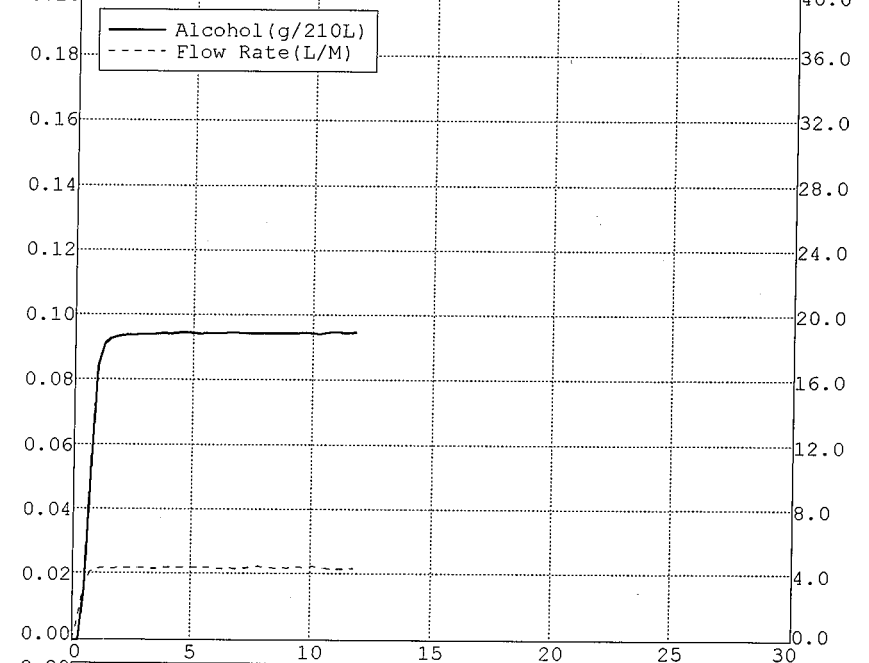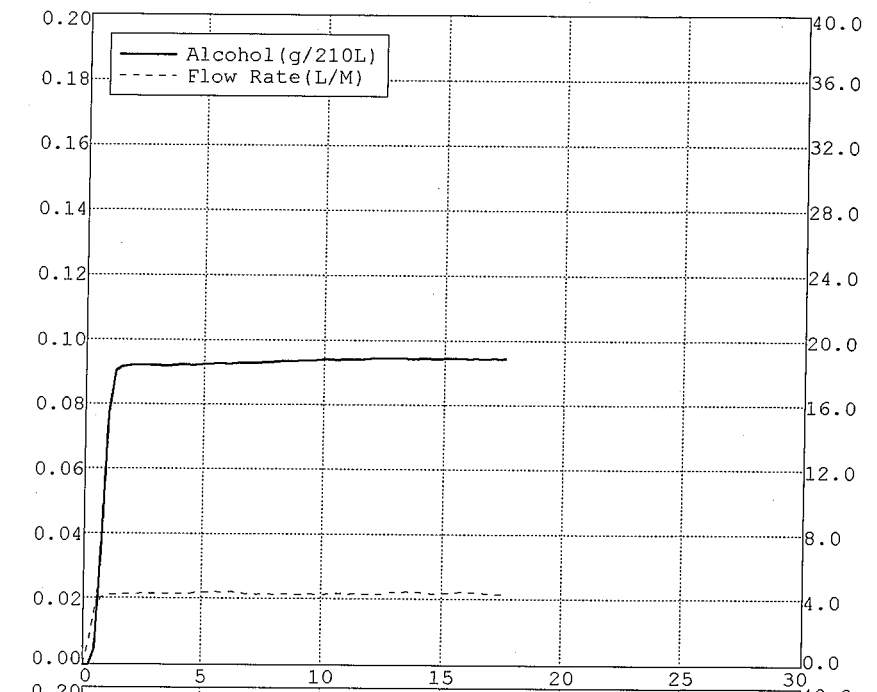

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 06/09/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:19
INTERNAL STANDARD	VERIFIED	10:19
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:20
BLANK TEST	0.00	10:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:21
BLANK TEST	0.00	10:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:22
BLANK TEST	0.00	10:23

26-22984

