

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282



Date: 06/23/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:30
INTERNAL STANDARD	VERIFIED	08:30
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:31
BLANK TEST	0.00	08:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:32
BLANK TEST	0.00	08:33
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:33
BLANK TEST	0.00	08:34

26-24700

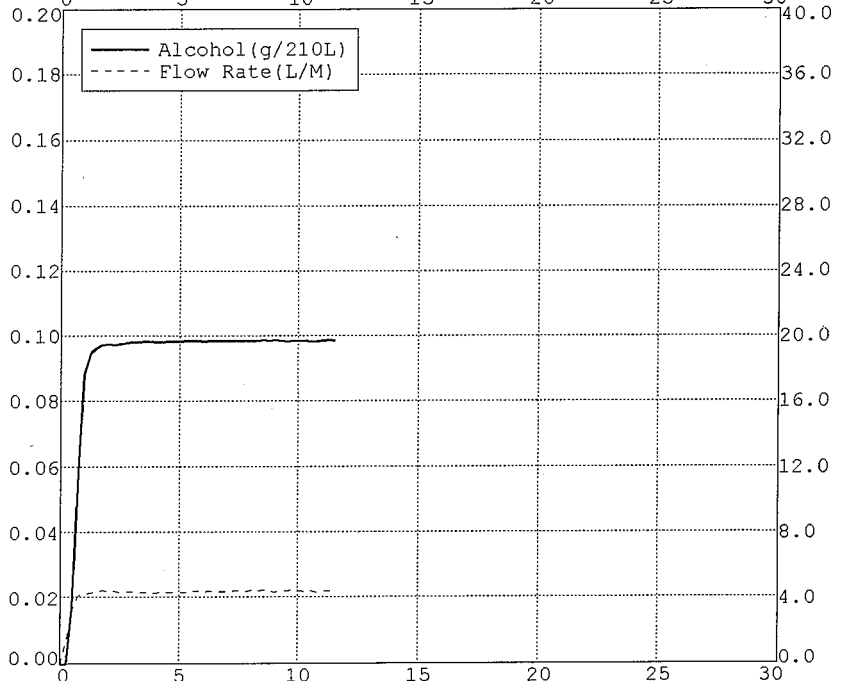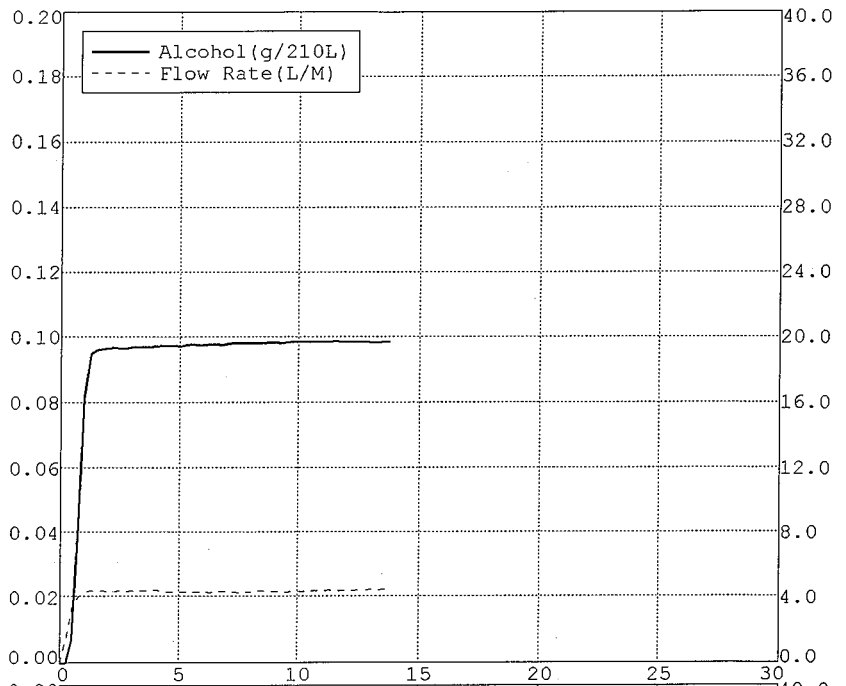

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 06/23/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:36
INTERNAL STANDARD	VERIFIED	08:36
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:37
BLANK TEST	0.00	08:37
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:38
BLANK TEST	0.00	08:38
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:39
BLANK TEST	0.00	08:40

26-24700

