

SUPERVISOR TEST

-----  
UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 107308  
-----




Date: 06/30/2026

OPERATOR NAME:  
JOSHUA R HARRINGTON  
Permit #: 38303  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:59
INTERNAL STANDARD	VERIFIED	08:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:59
BLANK TEST	0.00	09:00
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:00
BLANK TEST	0.00	09:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:01
BLANK TEST	0.00	09:02

26-25-599

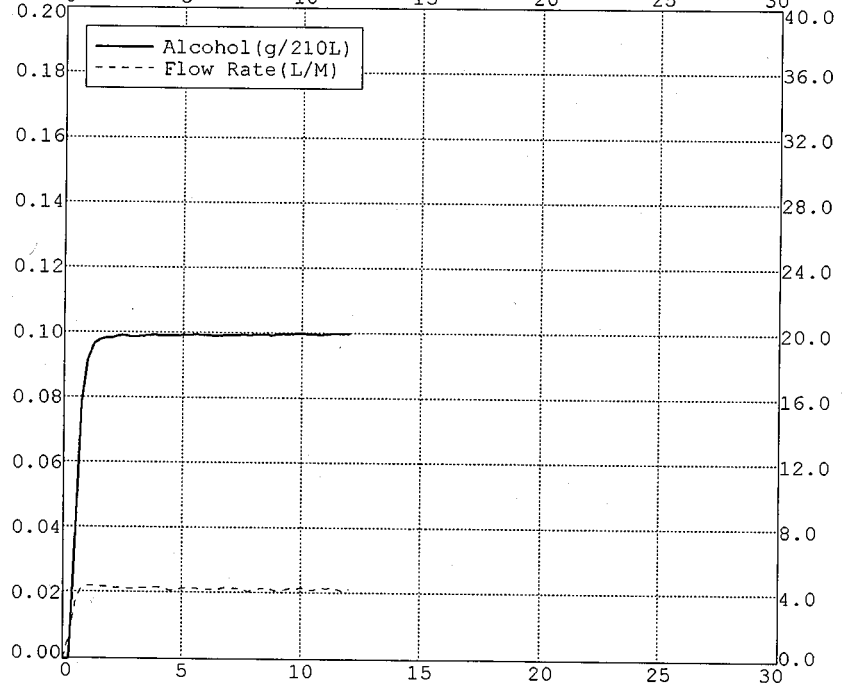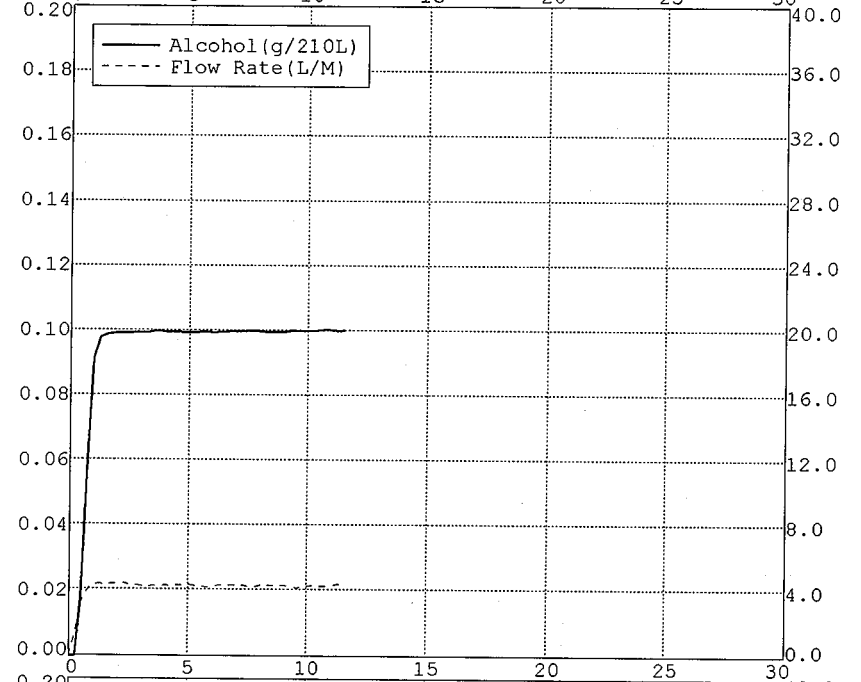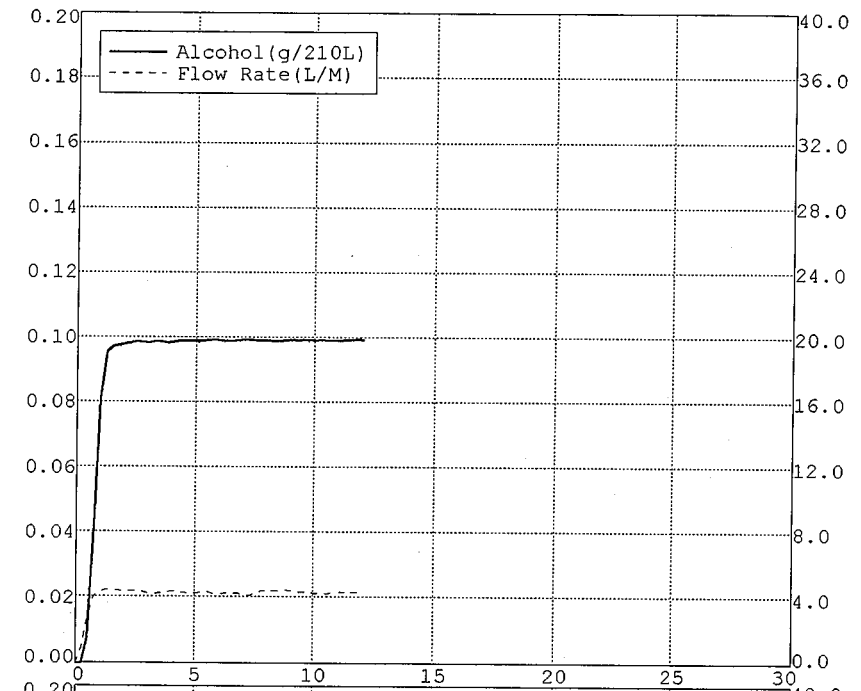

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 100282

Date: 06/30/2026

OPERATOR NAME:  
JOSHUA R HARRINGTON  
Permit #: 38303  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:44
INTERNAL STANDARD	VERIFIED	08:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:44
BLANK TEST	0.00	08:45
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:46
BLANK TEST	0.00	08:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:47
BLANK TEST	0.00	08:47

26-25599

