

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308



Date: 07/07/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:44
INTERNAL STANDARD	VERIFIED	11:44
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:45
BLANK TEST	0.00	11:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:46
BLANK TEST	0.00	11:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:47
BLANK TEST	0.00	11:48

26-27202

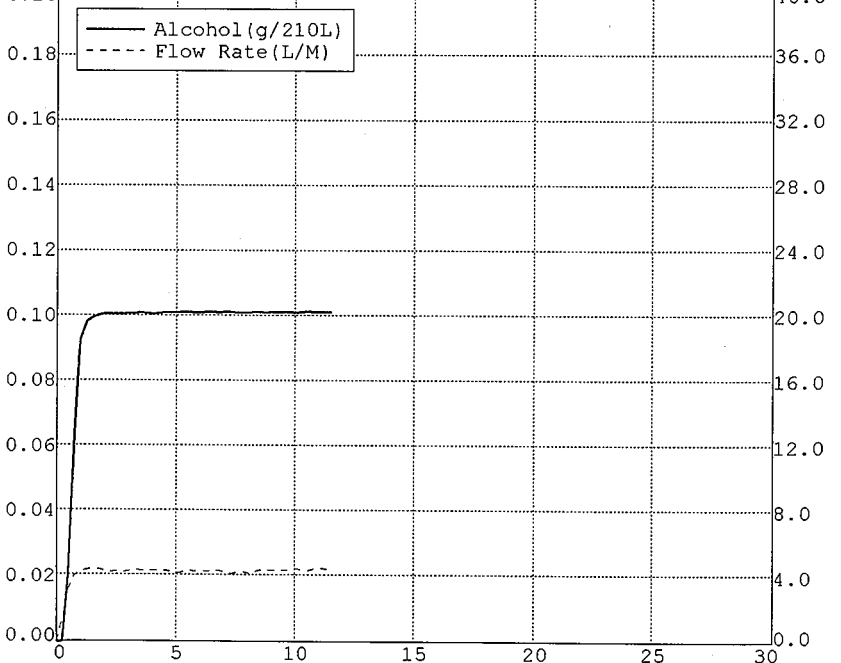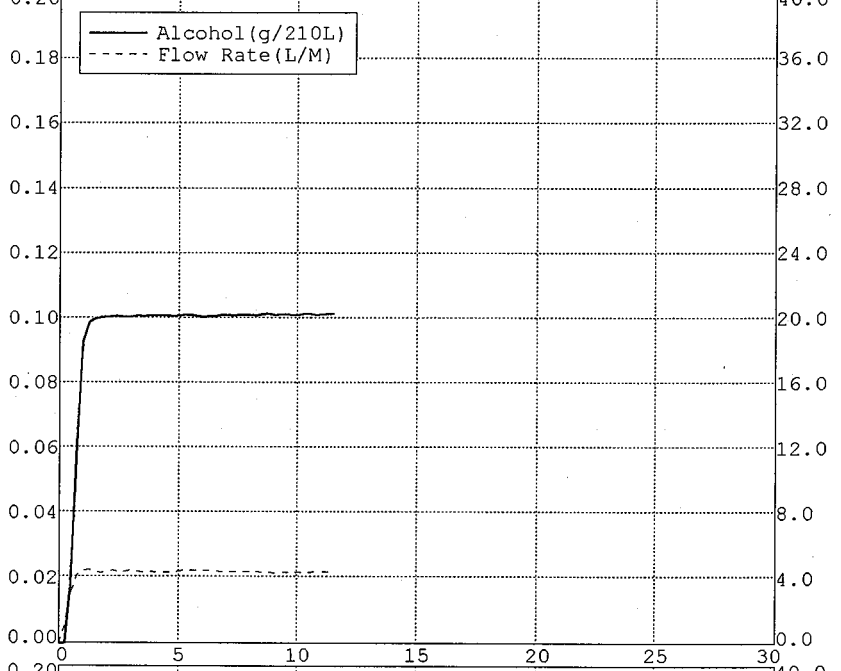

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 07/07/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:29
INTERNAL STANDARD	VERIFIED	11:29
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:30
BLANK TEST	0.00	11:30
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:31
BLANK TEST	0.00	11:32
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:32
BLANK TEST	0.00	11:33

26-27202

