

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 08/17/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:00
INTERNAL STANDARD	VERIFIED	08:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:01
BLANK TEST	0.00	08:01
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:02
BLANK TEST	0.00	08:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:03
BLANK TEST	0.00	08:04

26-33033

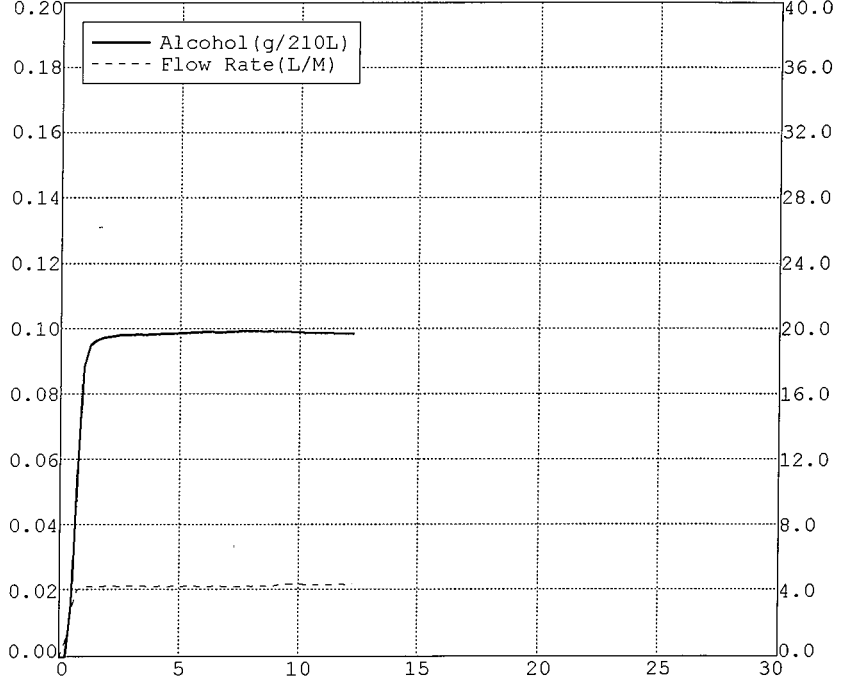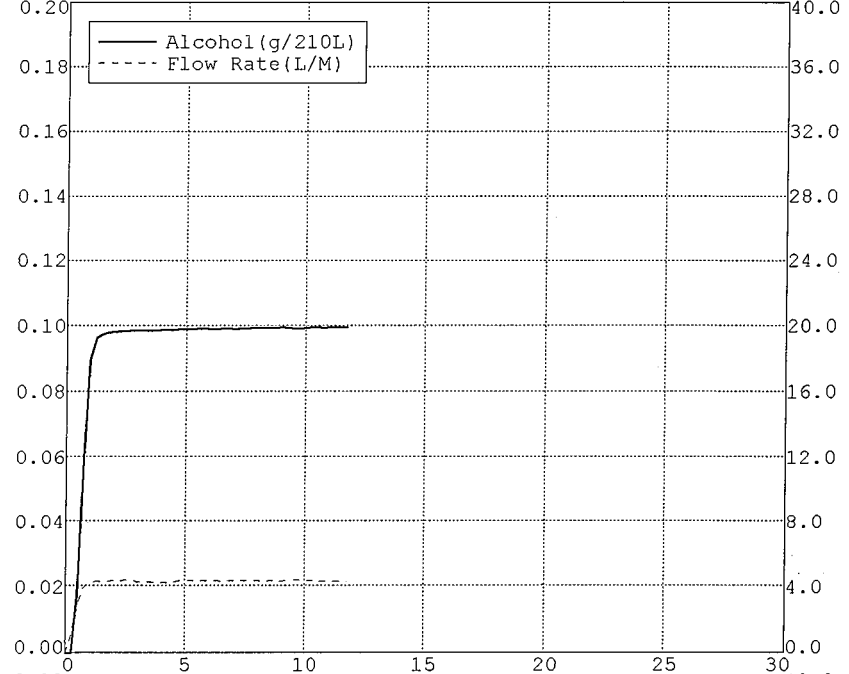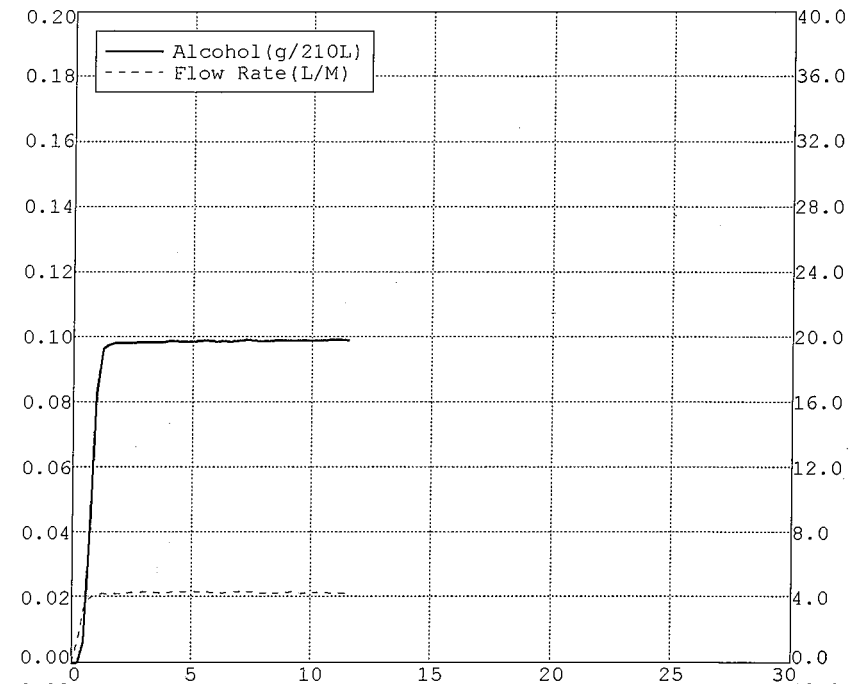

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 08/17/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:11
INTERNAL STANDARD	VERIFIED	08:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:11
BLANK TEST	0.00	08:12
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:12
BLANK TEST	0.00	08:13
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:13
BLANK TEST	0.00	08:14

26-33033

