

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 08/25/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:51
INTERNAL STANDARD	VERIFIED	11:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:51
BLANK TEST	0.00	11:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:52
BLANK TEST	0.00	11:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	11:53
BLANK TEST	0.00	11:54

26-36356

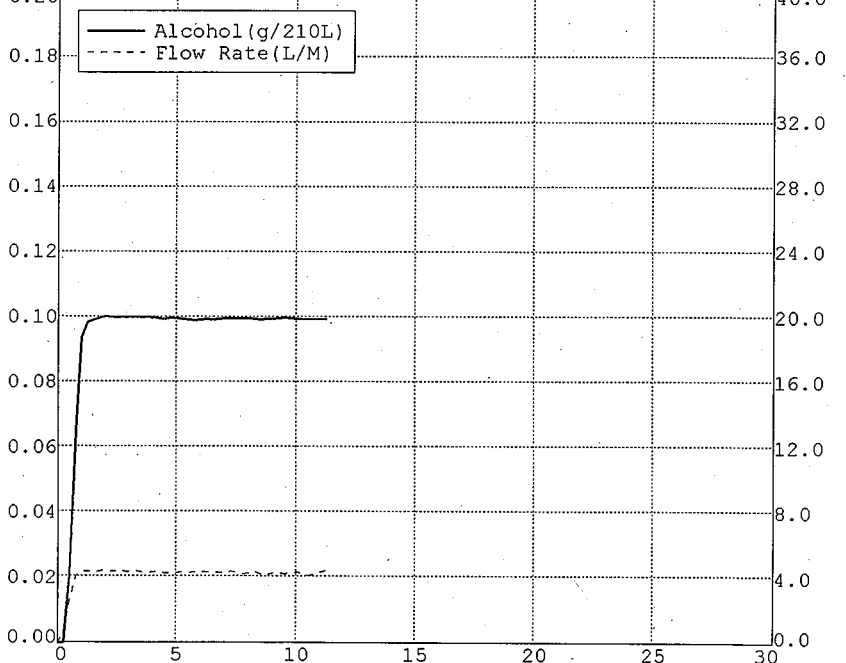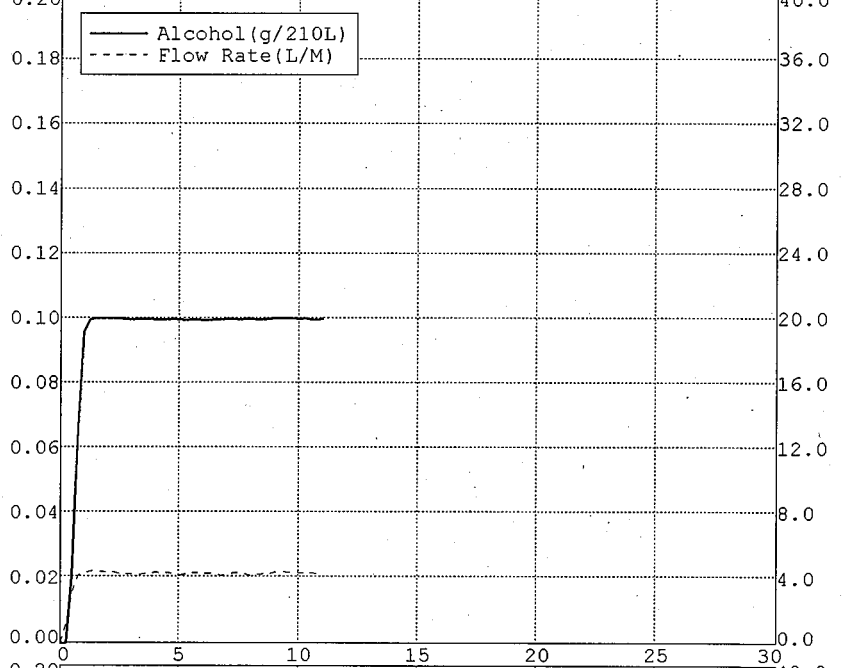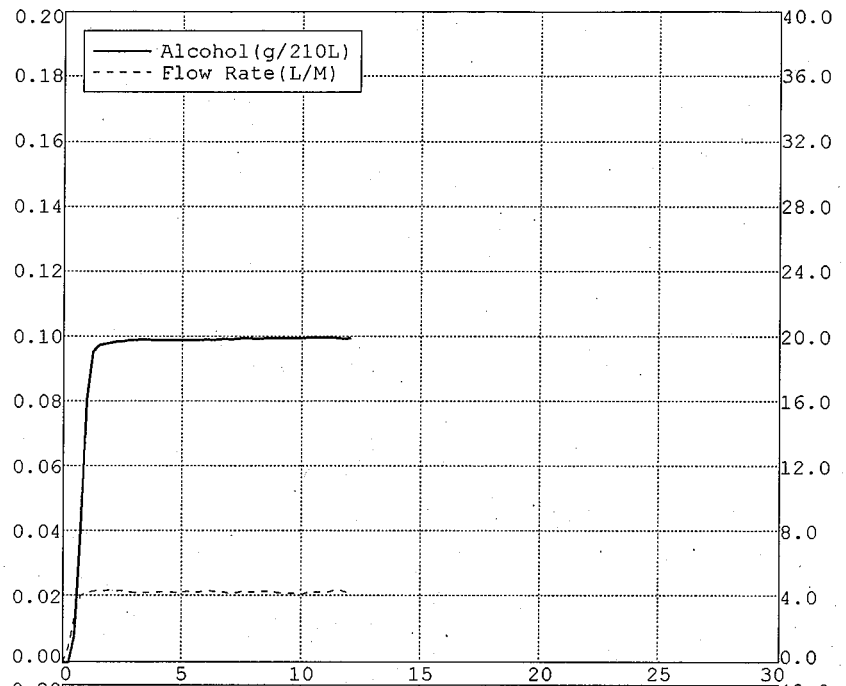

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 08/25/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:43
INTERNAL STANDARD	VERIFIED	11:43
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:43
BLANK TEST	0.00	11:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:44
BLANK TEST	0.00	11:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:45
BLANK TEST	0.00	11:46

26-36356

