

SUPERVISOR TEST

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308


Date: 09/08/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:41
INTERNAL STANDARD	VERIFIED	10:41
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:41
BLANK TEST	0.00	10:42
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:42
BLANK TEST	0.00	10:43
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:44
BLANK TEST	0.00	10:44

26-36545

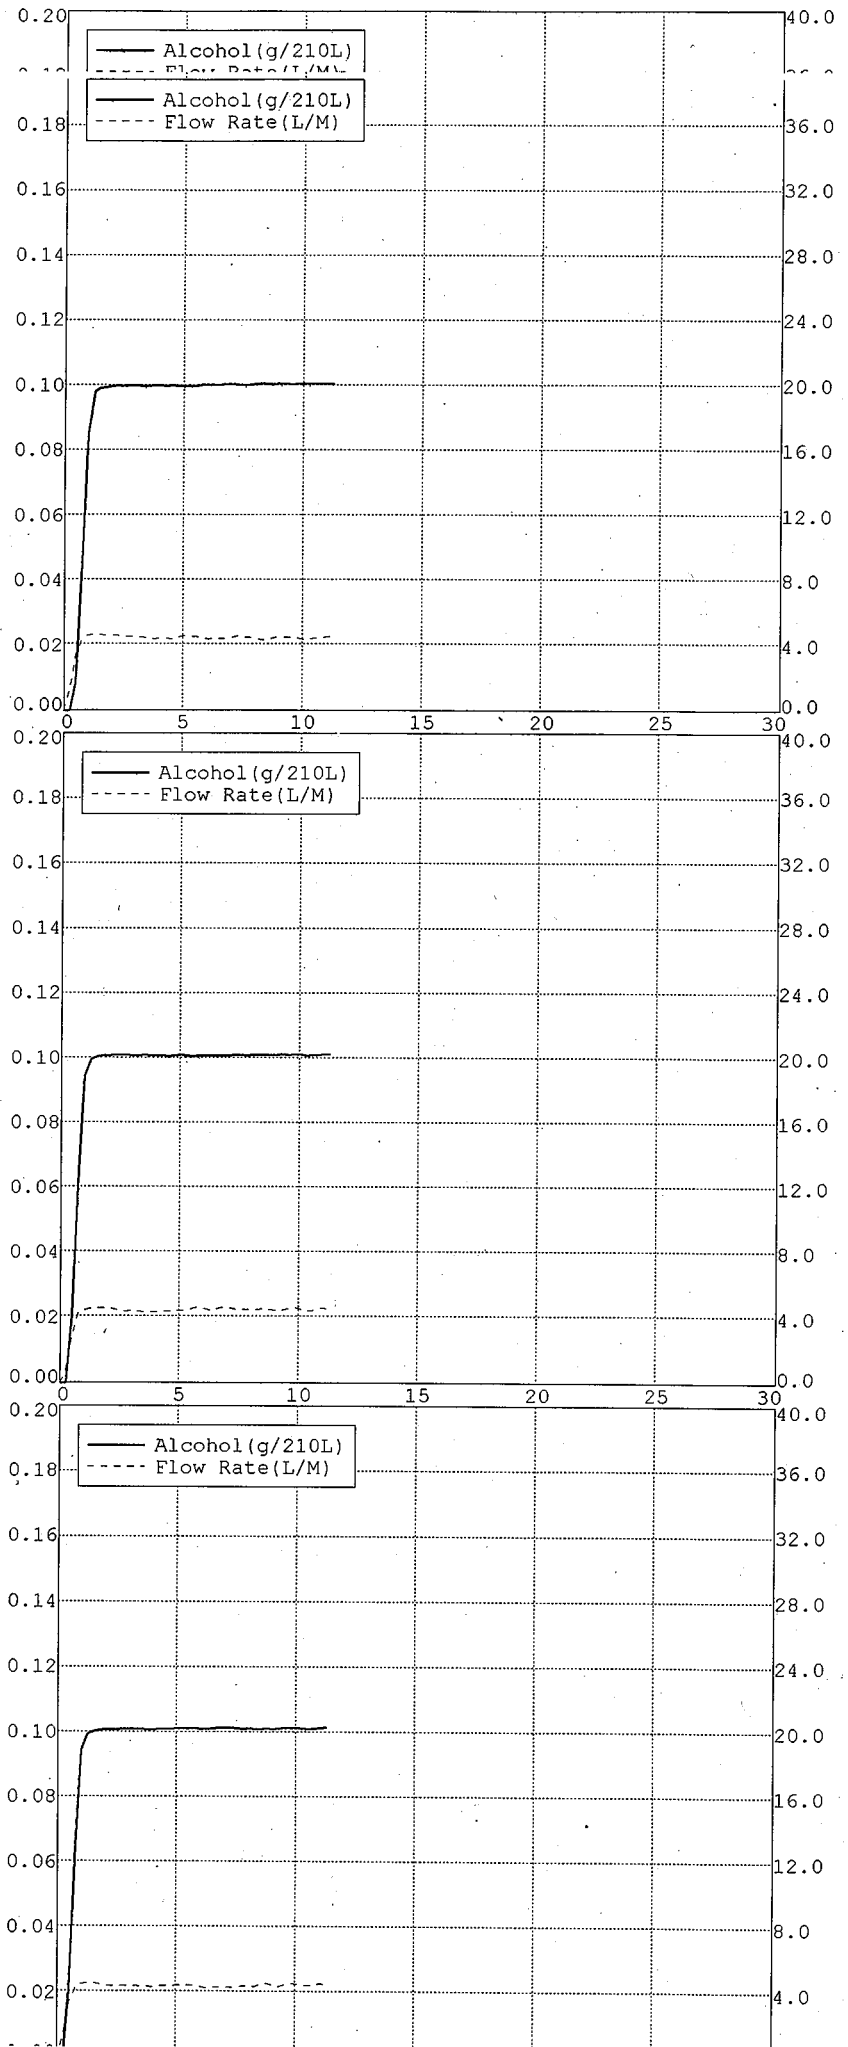

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 09/08/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:34
INTERNAL STANDARD	VERIFIED	10:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:34
BLANK TEST	0.00	10:35
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:35
BLANK TEST	0.00	10:36
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:36
BLANK TEST	0.00	10:37

26-36545

