

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 01/27/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25330

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:20
INTERNAL STANDARD	VERIFIED	10:20
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:20
BLANK TEST	0.00	10:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:21
BLANK TEST	0.00	10:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:22
BLANK TEST	0.00	10:23

Rms 26-3451

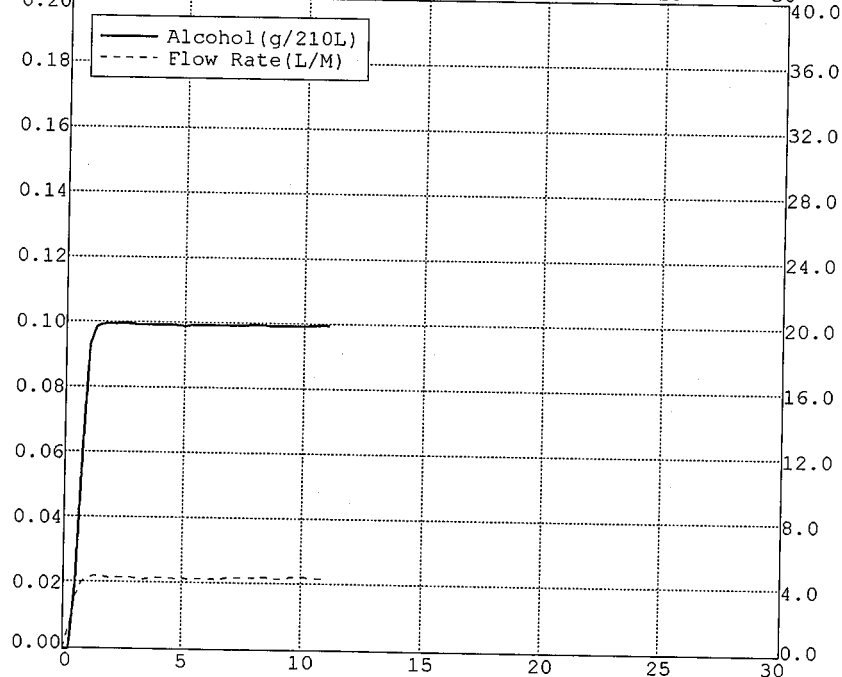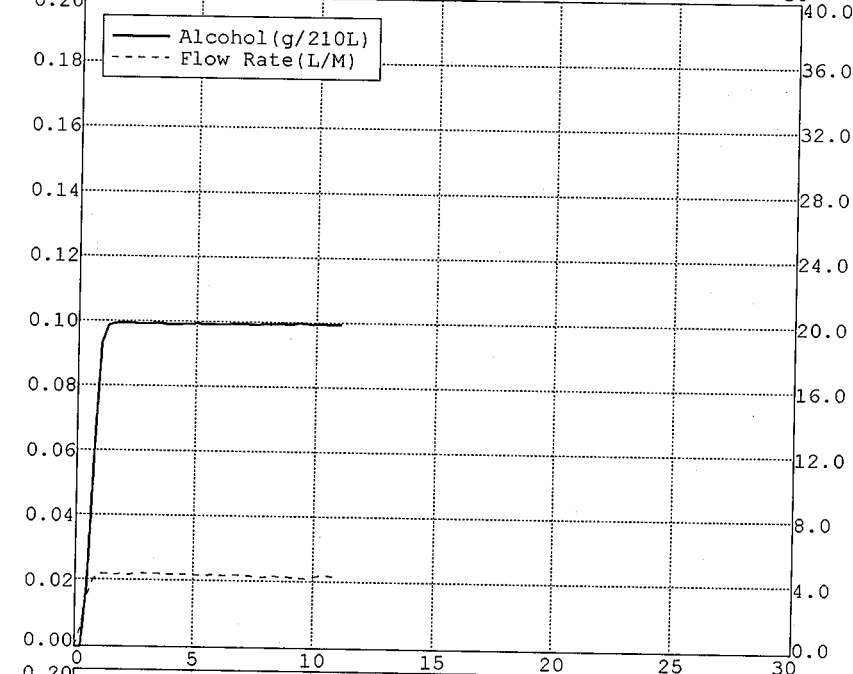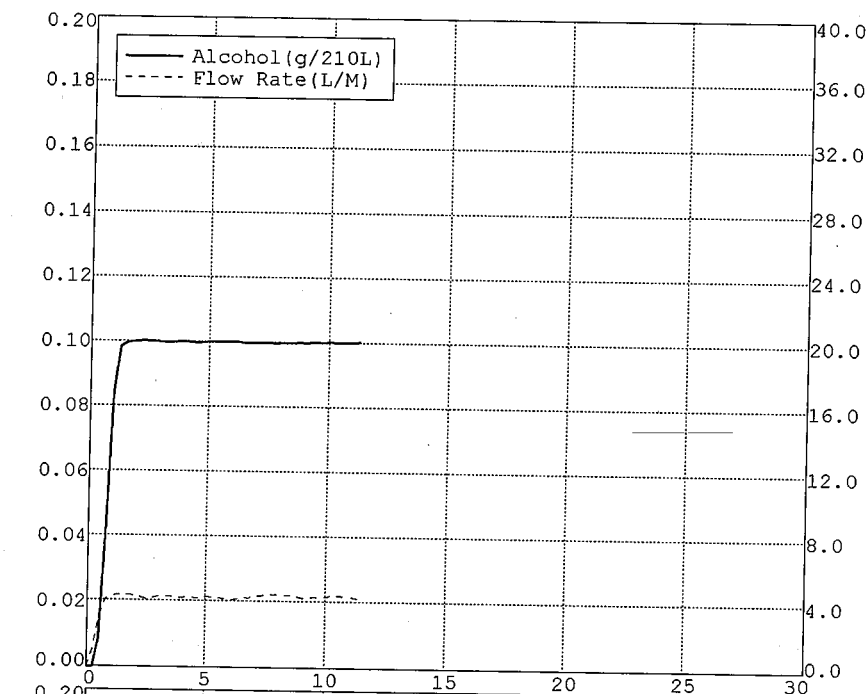

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 01/27/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25330

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:20
INTERNAL STANDARD	VERIFIED	10:20
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:20
BLANK TEST	0.00	10:21
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:21
BLANK TEST	0.00	10:22
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:22
BLANK TEST	0.00	10:23

RMS 26-3451

